



Status and developments of the shielding studies for the dummy septum TPS15

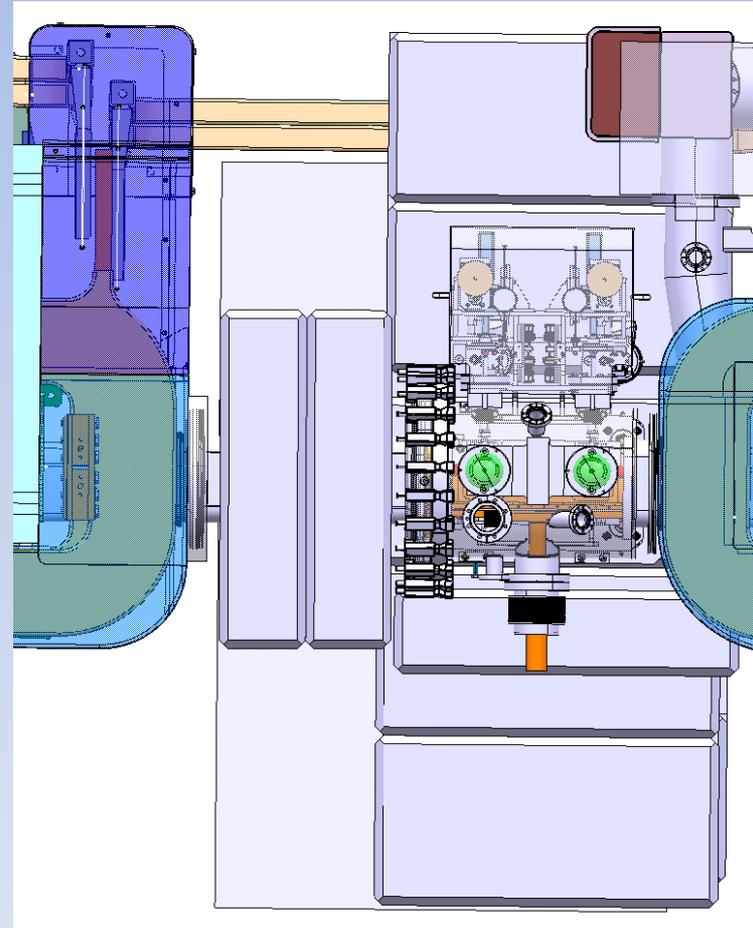

DANGER RADIATION 
SEJOUR LIMITE
OCCUPANCY TIME LIMITED
Before starting work contact 70488
50 µS/h
d'ambiance 7h/8

Downstream shielding dedicated to the vacuum chamber. In event of removal of dummy 15, top blocks only need to be removed.

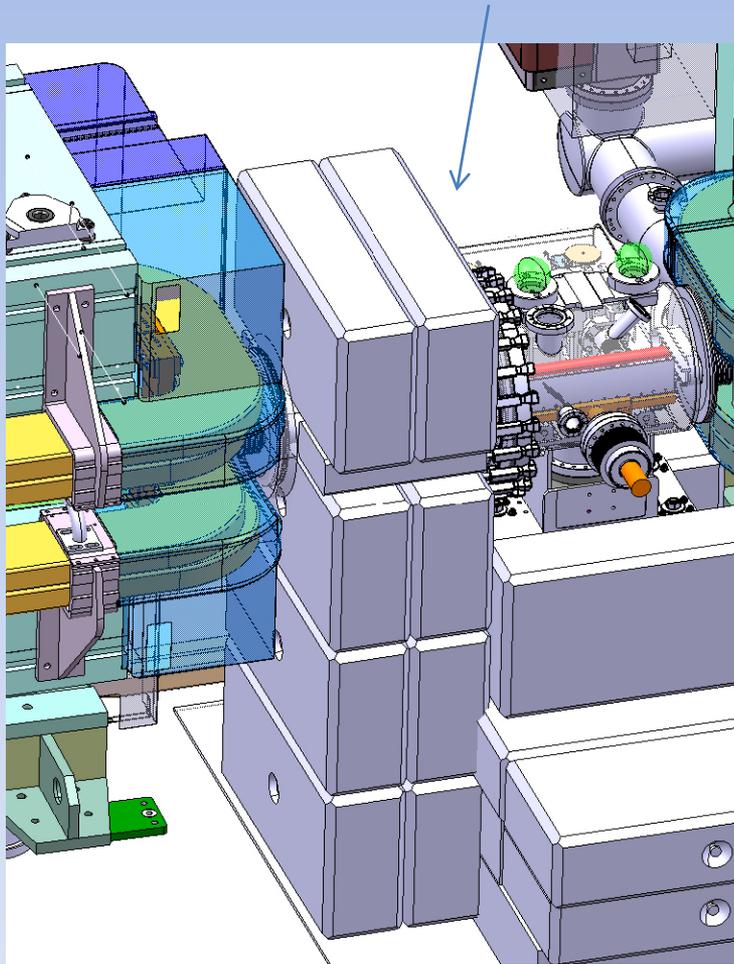

All standard blocks 800x400x200, No. required 8

Provisional requirements

Size	Quantity	Location		
800x400x200	8	Downstream Chamber		